

Rack Mount/Table Top NMGOC Analyzer Heated FID 109A

© J.U.M. Engineering 2014/2016

The 109A is a rack mount and table top heated emission analyzer for the continuous / simultaneous determination of the mass concentration of Non Methane Gaseous Organic Carbon using the Dual Flame Ionization Detector method. Throughout the EU the TGOC (TVOC) channel fully with complies with QAL1 (EN 14181-EN ISO 14659) and EN 12619:2013. In the USA full compliance with EPA Method 25A and Method 503



****Low cost of ownership. **Low fuel gas consumption.
The combustion air supply for the FID-detector is built in. No external cylinder for synthetic air is needed. **To prevent well known HC hang up (memory effect) and related drifting, the heated sample line can easily be connected inside of the heated oven. This prevents any cold spot and any related HC condensation

General:

The THC (TVOC) circuit of this analyzer fully complies with QAL1 (EN 14181-EN ISO 14659), with EN 12619:2013 and in USA with EPA Method 25A and Method 503

The 109A is the only available heated non methane gaseous organic carbon NMGOC (NMHC) FID-analyzer with an internal permanently installed sample filter to be cleaned by pack purge with compressed air or nitrogen. This feature cleans the sample filter and sample line at the same time. A stack filter probe is not required when the analyzer is used as a "stand alone", or the stack probe is equipped with a solenoid valve to allow the back purged contamination to be vented downstream of the stack filter. This makes the 109A ideal for CEM applications with extremely low sample line drift (hang up)

The J.U.M. Engineering HFID Model 109A is time proven in nearly 20 years. It is a highly reliable and outstandingly rugged 19" rack mount or table top heated NMGOC (non methane gaseous organic carbon) analyzer. Built for very low drift, high accuracy, sensitivity and stability. The 109A uses two parallel operating hydrogen flame ionization detectors (FID) in a heated oven to prevent the loss of high molecular weight hydrocarbons and to provide reliable performance in the analysis of high concentrations down to very low trace concentration levels of gaseous organic carbon contaminants in emissions, air and other gases and high purity gases. One of the two sample capillaries is connected in series to a temperature controlled catalyst module. This catalyst oxidizes all hydrocarbons except Methane carbon. Both detectors are connected to two individual electrometer amplifiers. From these two FID signals, total organic gaseous carbon from the detector without the catalyst and methane carbon from the detector with the catalyst, the non methane organic carbon signals is generated via differential calculation Thus resulting in the three continuous simultaneous signals shown on individual front panel displays. Three individual DC voltage and 4-20 mA signals are available in the rear panel plus an optional RS 232 data output per signal. All sample containing parts and components are discretely integrated into the heated chamber. The permanent heated sample filter is cleaned by back purging with compressed air or nitrogen. This allows uninterrupted measurements during cleaning the sample filter. While back purging the sample filter, the external sample line and sample probe is also cleaned. The use of a stack probe filter is not necessary when the FID is used in a stand alone mode. The combustion air supply for the detector is built in. No expensive zero gas generator or external cylinder for synthetic air is needed. The proprietary rear panel sample line adapter-plate system allows cold-spot free coupling of a heated sample line inside of the heated oven without the need of special tools. The fittings can easily be accessed through a wrench port in the right side panel.



Analyzer Features

- Made in Germany
- **1st Sampling Choice:** Maintenance free, permanently installed sample filter back purge system allows filter to be cleaned without dismantling (automatic back purge optional)
- **2nd Sampling Choice:** Disposable sample filter which is easily accessible in the rear panel without special tools. This optional available feature reflects a 20% price advantage.
- All components in contact with sample are fully heated and digitally maintained at 190°C
- Built-In sample pump
- Built-in combustion air supply, no extra burner air bottle needed
- Permanent 2 micron stainless steel wire mesh back purge sample filter or 2 micron disposable sample filter
- "Overflow" calibration system for safe zero and span calibration
- Automatic flame out alarm contact and optional available fuel shut off valve
- Fast response time
- Low fuel consumption @ 100% H₂ or 40/60 mixed fuel gases
- Microprocessor PID type temperature controller
- Cold spot free coupling of a heated sample line inside the heated oven with optional Adapter Plate (not available with OVE Option)
- Remote control for sample, zero gas, span gas and back purge is standard
- Automatic or remote range change optional


Applications

- Compliance monitoring of source total organic gaseous carbon, methane carbon and non methane organic gaseous carbon and with US EPA Method 25A and US IACA TCM-042
- VOC compliance stack emissions monitoring Industrial printing press dryer systems
- US EPA VOC compliance testing of bakery stack emissions
- Optimizing industrial bakery ovens
- Fence line (perimeter) monitoring
- Solvent recovery monitor for carbon bed break through
- Catalytic converter monitoring/ testing
- Thermal combustor monitoring/ testing
- Carbon adsorption regeneration monitoring and control
- Raw exhaust vehicle emissions analysis
- Hydrocarbon contamination monitoring in air and other gases


Principle of Operation

The Heated Flame Ionization Detection (HFID) method is used to determine the presence of total organic carbon concentrations in gaseous samples. Two detectors are used in parallel, one for TGOc and one for Methane Carbon (MC). Burning hydrocarbon-free hydrogen in hydrocarbon-free air produces a negligible number of ions in the detector. Once a sample which contains any organic carbon matter is introduced into this flame, a very complex ionization process is started. This process creates a large number of ions. A high polarizing voltage is applied between the two electrodes around the burner nozzle and produces an electrostatic field. Now negative carbon ions migrate to the collector electrode and positive hydrogen ions migrate to the high voltage electrode. The so generated ionization current between the two electrodes is directly proportional to the hydrocarbon concentration in the sample that is burned by the flame. This signal is measured and amplified by a highly sensitive and stable electro-meter-amplifier unit.


Our proprietary sample pressure regulator provides a controlled sample pressure and flow which gives admittance of a constant sample flow rate to the FID burner. This technique of using our non sample contact regulator is time proven for over 40 years by J.U.M. Engineering to provide the highest possible sample low flow rate stability at the lowest maintenance. Our compactly designed flow control module for fuel, ignition and air flow rates via low thermal mass needle valves use high precision pressure regulators. The needle valves are factory adjusted and sealed to ensure the optimization of the burner.

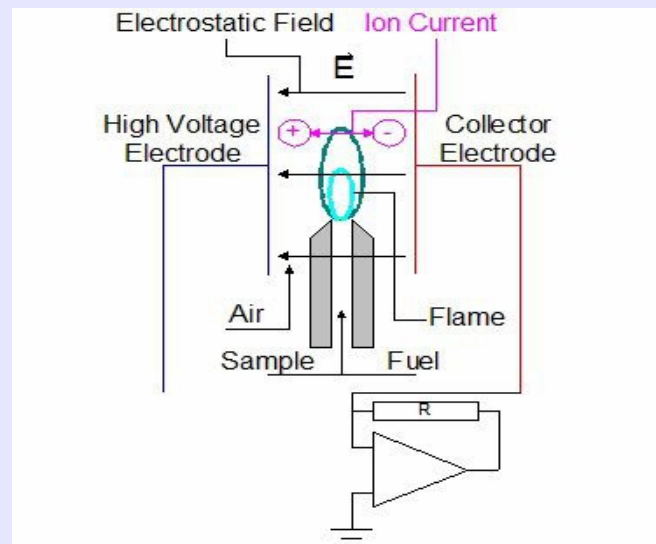

109A Heated FID Total Continuous Gaseous NMGOC Analyzer

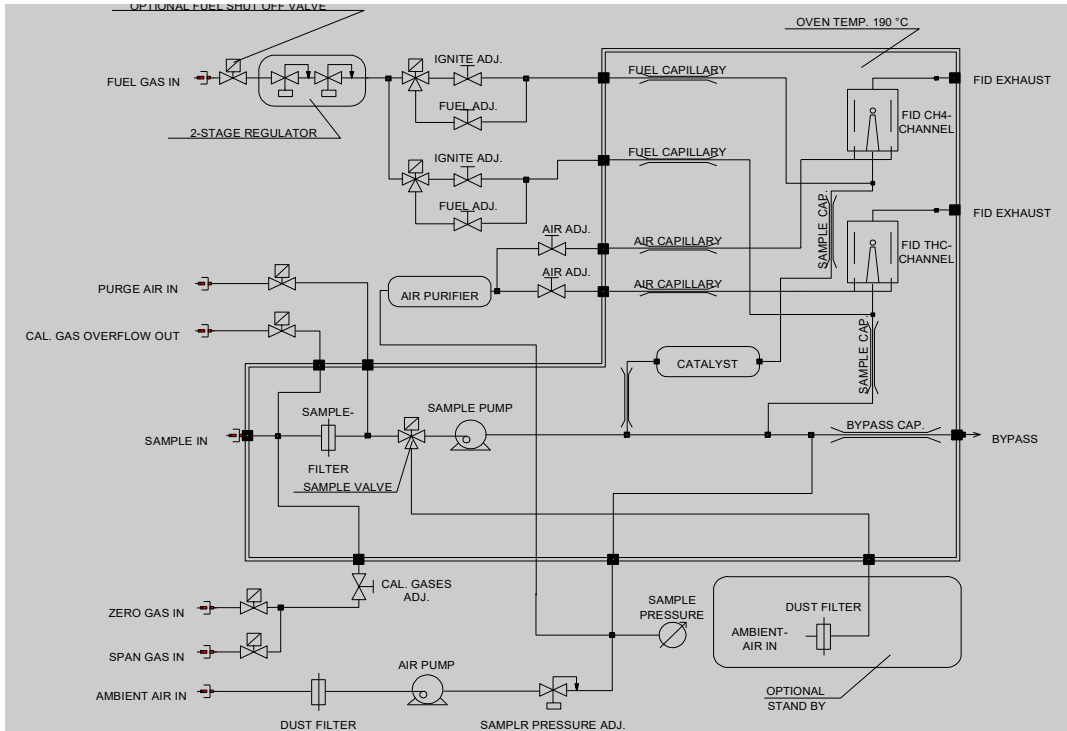

Complete flow diagram shown with standard back purge sample filter

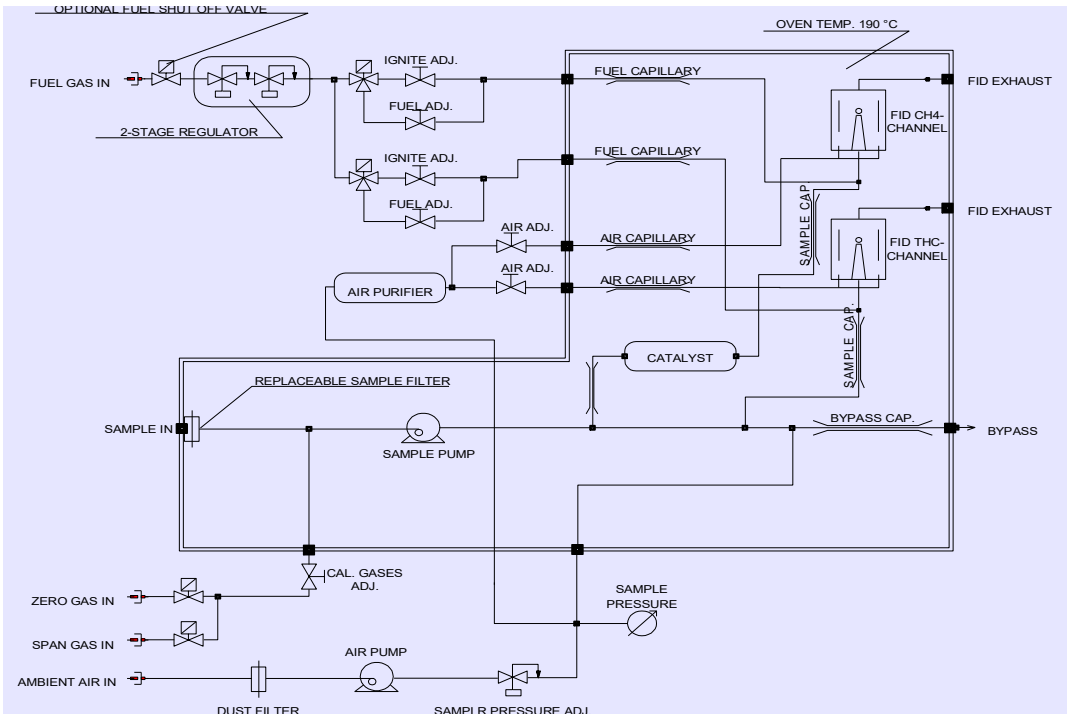

Complete flow diagram shown with alternative disposable sample filter Option OVE 9



Technical Specifications

Method	Dual heated Flame Ionization Detector (HFID) one for TGOC, one for MOC (CH ₄)
Sensitivity	Max. 1 ppm CH ₄ full scale
Response time TGOC	<0.2 seconds @ sample inlet
Response time CH₄	< 15 seconds @ sample inlet
T₉₀ time TGOC	< 1.2 seconds @ sample inlet
T₉₀ time CH₄	< 50 seconds @ sample inlet
Linearity	Up to 10.000 ppm full scale within 1.5%
Oxygen synergism	< 2.5% FSD
Measuring ranges (ppm)	0-10, 100, 1,000, 10,000, 100,000, others on request. Front panel turn switch, automatic or remote control optional
Signal outputs	One each 0-10 VDC, 4-20 mA, RS-232 data output for TGOC, MGO and NMGOC and
Display	6- digit direct reading ppm units capability to measure 3 overlapping ranges without range change
Total sample flow through	2.5 to 2.8 l/min capacity @ operating temp.
Sample filter	Permanent 2 micron mesh filter, cleaned by back purge with compressed dry air or N ₂ . Alternatively disposable change filter in rear panel. Option OVE 9
Zero and Span gas	Front panel switch selectable and remote control, gas inlets on rear panel
Zero and span adjust	Manual duo dials on front panel
Fuel gas choice	<ol style="list-style-type: none"> 1. Standard 100% H₂, consumption approx. 40 ml/min 2. Optional 40%H₂/60%He, consumption approximately 180 ml/min 3. Optional 40%N₂/60%He, consumption approximately 180 ml/min
Burner air consumption	Built in burner air supply. No external cylinder air needed. consumption approximately 260 ml/min. At 40/60 mixed fuels. Air consumption is approx. 450 ml/min
Oven temperature	190 °C (374 °F)
Temperature control	micro-processor PID controller
Power requirements	230VAC/50Hz, 900 W. 120 VAC/60Hz optional
Ambient temperature	5-43 °C (41-110 °F)
Dimensions (W x D x H)	19" (483 mm) x 460 mm x 221 mm
Weight	approx. 24 kg (50 lbs)

Available Options

OVE 9	Quick change, disposable 2 micron sample filter housed in the heated oven in stead of back purge sample filter (A 20% Price Advantage)
OWM 9 *	Wall or panel mount adapted system allows the analyzer to be installed on a wall, a panel, or inside of an outdoor or safety purged enclosure. Includes extractive FID exhaust. Only available on special request.
AMU 9	Automatic controlled range change with range identification
APO 9	Automatic sample filter pack purge; Internal, easily programmable back purge timing system for back purge time and purge sequence sequence
AZM 9	Automatic flame ignition and re-ignition
ENGA 9	6-digit engineering units display 0-100.000 ppm (or others) with RS232 data output. 24 bit resolution allows to digitally measure throughout 2 to 3 measuring ranges without range change
FOAS 9	Flame out control with automatic fuel shut off valve
MBP 9	Integrated bypass pump for very long sample lines, also compensates sample pressure fluctuations at sample inlet. Not available with PDA option
PDA 9	Sample pressure monitor with alarm
RCC 9	Remote controlled range change with range identification (dry contact)
RCI4 9	4-20 mA analog output, galvanic isolated
RCIO 9	0-20 mA analog output, galvanic isolated
TPR 9	External temperature controller for J.U.M. heated sample lines TJ 100 or other brand with "J" type thermocouple

Important! * When equipped with OWM option the analyzer design is to be mounted upright with all gas and electrical connections on top. The dimensions are (W x D x H) 383 mm (19") x 221 mm x 700 mm

J.U.M.® Engineering GmbH

Gauss-Str. 5, D-85757 Karlsfeld, Germany

Tel.: 49-(0)8131-50416, Fax: 49-(0)8131-98894

E-mail: info@jum.com

Internet: www.jum-aerosol.com

1st Published: Nov. 2014, Print: March 2016